

Primerdesign Ltd

SNPsig[®] SARS-CoV-2 (20I/501Y.V1)

UK variant

SNPsig[®] real-time PCR
SARS-CoV-2 mutation detection/
allelic discrimination kit

96 tests

For general laboratory and research use only

Kits by Primerdesign

Kit contents

- **SARS-CoV-2_20I/501Y.V1 genotyping primer/probe mix (labelled A1708D, 96 reactions **BROWN**)**
FAM and HEX labelled
- **Wild-type positive control template (**RED**)**
- **Mutant positive control template (**RED**)**
- **RNase/DNase free water (**WHITE**)**
for resuspension of primer/probe mix
- **Template preparation buffer (**YELLOW**)**
for resuspension of positive control templates
- **oasig[®] Lyophilised OneStep 2X RT-qPCR Mastermix (**RED**)**
contains complete Onestep RT-qPCR mastermix
- **oasig[®] resuspension buffer (**BLUE**)**
for resuspension of the lyophilized mastermix

Reagents and equipment to be supplied by the user

Real-time PCR Instrument

Must be able to read fluorescence through FAM and HEX channels

Pipettes and tips

Vortex

Centrifuge

Suitable qPCR 96W plates or qPCR reaction tubes

Kit storage and stability

This kit is stable at room temperature but should be stored at -20°C on arrival. Primerdesign does not recommend using the kit after the expiry date stated on the pack. Once the lyophilised components have been resuspended, unnecessary repeated freeze/thawing should be avoided. The kit is stable for six months from the date of resuspension under these circumstances.

Suitable sample material

SNPsig SARS-CoV-2 A1708D is intended for use as a **reflex test** only. Thus, a primary confirmation test for SARS-CoV-2 would be carried out using suitable methodology, and the extracted RNA from patient samples (or any material suited for PCR amplification) thereafter applied to this test. Please ensure that the samples are suitable in terms of purity, concentration, and RNA integrity. Always run at least one negative control with the samples. To prepare a negative control, replace the template RNA sample with RNase/DNase free water.

Notices and disclaimers

This product is developed, designed and sold for research purposes only. It is not intended for human diagnostic or drug purposes or to be administered to humans unless clearly expressed for that purpose by the Food and Drug Administration in the USA or the appropriate regulatory authorities in the country of use. During the warranty period Primerdesign snpsig detection kits allow precise and reproducible data recovery combined with excellent sensitivity. For data obtained by violation to the general GLP guidelines and the manufacturer's recommendations the right to claim under guarantee is expired. PCR is a proprietary technology covered by several US and foreign patents. These patents are owned by Roche Molecular Systems Inc. and have been sub-licensed by PE Corporation in certain fields. Depending on your specific application you may need a license from Roche or PE to practice PCR. Additional information on purchasing licenses to practice the PCR process may be obtained by contacting the Director of Licensing at Roche Molecular Systems, 1145 Atlantic Avenue, Alameda, CA 94501 or Applied Biosystems business group of the Applied Biosystems Corporation, 850 Lincoln Centre Drive, Foster City, CA 94404. In addition, the 5' nuclease assay and other homogeneous amplification methods used in connection with the PCR process may be covered by U.S. Patents 5,210,015 and 5,487,972, owned by Roche Molecular Systems, Inc., and by U.S. Patent 5,538,848, owned by The Perkin-Elmer Corporation.

Trademarks

Primerdesign™ is a trademark of Primerdesign Ltd. The PCR process is covered by US Patents 4,683,195, and 4,683,202 and foreign equivalents owned by Hoffmann-La Roche AG. BI, ABI PRISM® GeneAmp® and MicroAmp® are registered trademarks of the Applied Biosystems (Applied Biosystems Corporation). BIOMEK® is a registered trademark of Beckman Instruments, Inc.; iCycler™ is a registered trademark of Bio-Rad Laboratories, Rotor-Gene is a trademark of Corbett Research. LightCycler™ is a registered trademark of the Idaho Technology Inc. GeneAmp®, TaqMan® and AmpliTaqGold® are registered trademarks of Roche Molecular Systems, Inc., The purchase of the Primerdesign reagents cannot be construed as an authorization or implicit license to practice PCR under any patents held by Hoffmann-La Roche Inc.

Introduction

The Novel Coronavirus Disease 2019 (COVID-19) pandemic, caused by SARS-CoV-2 virus, represents a major threat to health. COVID-19 has resulted in widespread morbidity and mortality. SARS-CoV-2 is known to have infected more than 90 million people (1). As the virus has spread across the world, mutations have arisen resulting in divergent clusters (clades) with different prevalence in different geographic regions (2,3).

One major clade to be identified is 20I/501Y.V1, also known as VOC202012/01 and B.1.1.7. This variant has been identified as approximately 70% more transmissible (4). This variant contains the N501Y replacement in the spike protein and has been shown to increase ACE2 binding (5). This variant has been seen with a 69-70 nucleotide deletion which has been shown to impact performance of some diagnostic PCR assays using an S gene target (6). In addition, this variant contains P681H which is located near a furin cleavage site and is believed to contribute to the increase in transmissibility (7,8). Recent independent analyses suggest that there might be a realistic possibility that infection with VOC 20I/501Y.V1 is associated with an increased risk of death compared to infection with non-VOC viruses (9).

501Y.V1 (or VOC202012/01) has now been detected in 60 countries, comprising all six WHO regions to date (10). Currently, authorities are using the occurrence of S gene target failure (SGTF) as a proxy for this strain. However, given the shared nature of these mutations and rising evidence for convergent evolution, tests are needed to define specific strains. Targeting of A1708D in ORF1B is 100% specific for this strain and will allow targeted testing of SGTF to determine the precise variant.

Principles of the test

Genotyping by real-time PCR using hydrolysis probes

Each genotyping primer/probe mix contains two labelled probes homologous to the two genotypes under investigation. During qPCR amplification of the reverse-transcribed target RNA, the probes will compete for binding across the variant region. The probe that is 100% homologous to the binding site will preferentially bind and give a fluorescent signal as PCR proceeds. It follows that the wild-type sequence will give a strong amplification plot through one channel whilst giving a very weak signal through the alternative channel. Homozygous variant samples will give an exactly inverse result. Most hardware platforms can perform this analysis automatically.

Positive controls

The kit contains positive control templates for each of the two genotypes. These can be run as parallel samples to give control signals for each genotype. In order to provide good positive control data that is directly relevant to the samples under test, the positive control template should be used at a similar copy number to the sample RNA. Positive control templates are a potential contamination risk to subsequent tests so must be handled carefully.

Negative control

To confirm the absence of contamination, a negative control reaction should be included every time the kit is used. In this instance, the RNase/DNase free water should be used instead of template RNA. A negative result indicates that the reagents have not become contaminated while setting up the run. If a positive result is obtained the results should be ignored and the test samples repeated. Possible sources of contamination should first be explored and removed.

Master mix compatibility

oasig[®] Lyophilised OneStep 2X RT-qPCR Master Mix contains the enzyme, nucleotides, buffers and salts at precisely the correct concentration for this application. The annealing temperatures of the primer and probe have been carefully calibrated and any change in the reaction buffer can significantly alter the performance of the assay. For this reason, Primerdesign can only guarantee accurate genotyping results when oasig[®] Lyophilised OneStep 2X RT-qPCR Master Mix is used.

Resuspension Protocol

To minimize the risk of contamination with foreign RNA, we recommend that all pipetting be performed in a PCR clean environment. Ideally this would be a designated PCR lab or PCR cabinet. Filter tips are recommended for all pipetting steps. The positive control template is a significant contamination risk and should therefore be pipetted after negative control and sample wells.

1. Pulse-spin each tube in a centrifuge before opening.

This will ensure lyophilised primer and probe mix is in the base of the tube and is not lost upon opening the tube.

2. Resuspend the primer/probe mix in the RNase/DNase free water supplied, according to the table below.

To ensure complete resuspension, vortex the tube thoroughly.

Component - Resuspend in water	Volume
SARS-CoV-2 A1708D primer/probe mix (BROWN)	110 µl

3. Resuspend the mastermix in resuspension buffer supplied, according to the table below.

Component - Resuspend in resuspension buffer	Volume
oasig [®] Lyophilised OneStep 2X RT-qPCR Mastermix (RED)	525 µl

4. Resuspend the positive control templates in the template preparation buffer supplied, according to the table below.

To ensure complete resuspension, vortex each tube thoroughly.

Component - Resuspend in template preparation buffer	Volume
Wild-type Positive Control Template (RED) *	500 µl
Mutant Positive Control Template (RED) *	500 µl

* This component contains high copy number template and is a VERY significant contamination risk. It must be opened and handled in a separate laboratory environment, away from the other components.

qPCR detection protocol

- 1. Prepare a complete genotyping reaction mix for the primer/probe mix according to the table below:**

Include sufficient reactions for all samples, positive and negative controls.

Component	Volume
oasig [®] OneStep 2X RT-qPCR Master Mix Lyophilised	10 µl
SARS-CoV-2 A1708D primer/probe mix (BROWN)	1 µl
RNase/DNase free water (WHITE)	4 µl
Final Volume	15 µl

- 2. Pipette 15µl of this mix into each well according to your qPCR experimental plate set up.**

- 3. Prepare RNA templates for each of your samples.**

As this is a reflex test, the RNA obtained from the confirmatory primary assay for SARS-CoV-2 should be used.

- 4. Pipette 5µl of RNA template into each well, according to your experimental plate set up.**

For negative control wells use 5µl of RNase/DNase free water. The final volume in each well is 20µl.

- 5. Dilute each positive control template in template preparation buffer.**

The positive control templates must each be diluted according to the table below:

Copies/reaction	Positive control dilution factor
10 ⁴	1:100

- 6. Pipette 5µl of each positive control RNA according to your experimental plate set up.**

qPCR amplification protocol

The following protocol is recommended for optimum resolution between genotypes:

Protocol for oasig[®] OneStep 2X RT-qPCR Master Mix

	Step	Time	Temp
	Reverse transcription	10 min	55 °C
	Enzyme activation	2 min	95 °C
Cycling x45	Denaturation	10s	95 °C
	Annealing and extension (DATA COLLECTION) *	60s	60 °C


* Fluorogenic data should be collected during this step through the **FAM** and **HEX** channels

Interpretation of results

The wild-type probe is labelled to read through the FAM channel whilst the mutant probe is labelled to read through the HEX channel. On wild-type sequences the FAM channel will give a strong amplification plot and the HEX channel none or very low detection. The signals are reversed on mutant samples. Cq values >40 should be disregarded and counted as inconclusive.


Sample data

Wild Type sample (**WT signal**, **Mutant signal**)

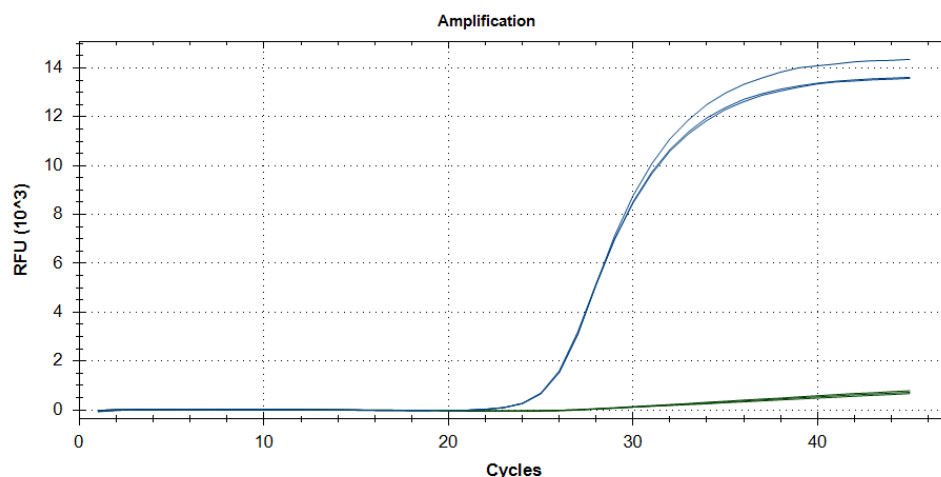


Amplification in the FAM (Blue) channel with no amplification in the HEX (green) channel indicates the presence of wild type template only.

Variant RNA sample (**WT signal**, **Mutant signal**)

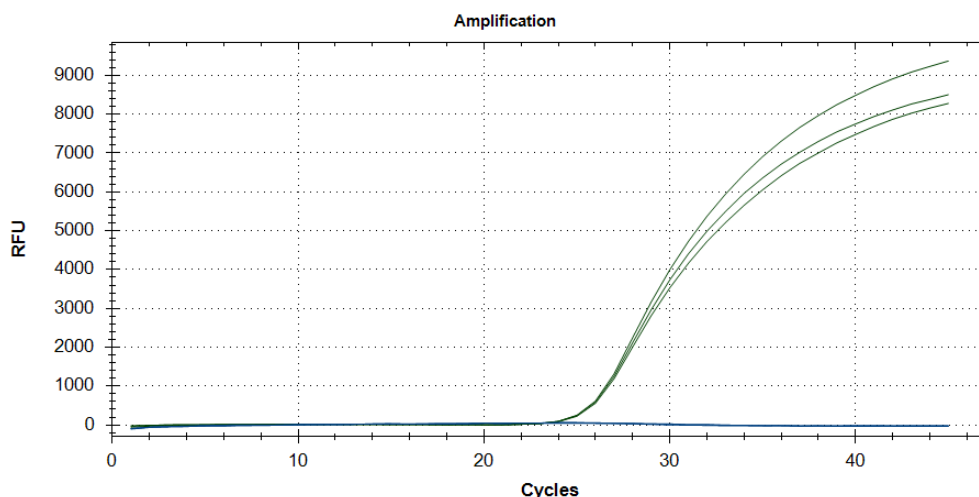

Amplification in the HEX (green) channel with no amplification in the FAM (blue) channel indicates the presence of mutant template only.

The raw data above can best be visualised by using a cluster analysis; plotting the end point fluorescence data from the FAM channel on one axis and the end point fluorescence data from the HEX channel on the other axis. Most qPCR software platforms will perform this analysis automatically so follow the manufacturer's instructions for your software. The data are quickly resolved into clusters corresponding to the wild-type, and mutant variant samples.

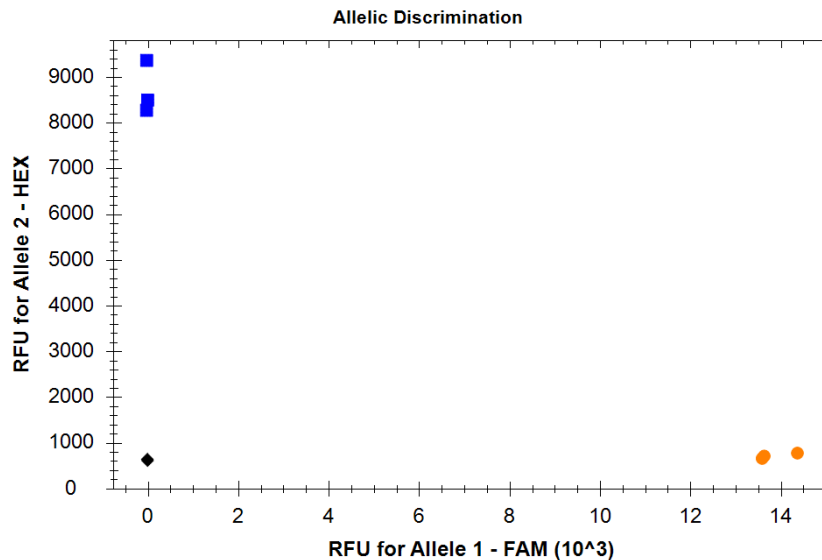

References

1. World Health Organisation (WHO). Coronavirus disease (COVID-19) [Internet]. [cited 2021 Jan 13]. Available from: <https://www.who.int/emergencies/diseases/novel-coronavirus-2019>
2. Hadfield J, Megill C, Bell SM, Huddleston J, Potter B, Callender C, et al. NextStrain: Real-time tracking of pathogen evolution. *Bioinformatics* [Internet]. 2018 [cited 2021 Jan 13];34(23):4121–3. Available from: <https://pubmed.ncbi.nlm.nih.gov/29790939/>
3. Tang X, Wu C, Li X, Song Y, Yao X, Wu X, et al. On the origin and continuing evolution of SARS-CoV-2 [Internet]. [cited 2021 Jan 13]. Available from: <https://www.who.int/emergencies/diseases/novel-coronavirus-2019/situation-reports/>
4. Hayward A, Shen Lim Julian Hiscox W, Edmunds J. NERVTAG meeting on SARS-CoV-2 variant under investigation VUI-202012/01. JVT; 2020 Nov.
5. Starr TN, Greaney AJ, Hilton SK, Ellis D, Crawford KHD, Dingens AS, et al. Deep Mutational Scanning of SARS-CoV-2 Receptor Binding Domain Reveals Constraints on Folding and ACE2 Binding. *Cell* [Internet]. 2020;182(5):1295-1310.e20. Available from: <http://dx.doi.org/10.1016/j.cell.2020.08.012>
6. WHO | SARS-CoV-2 Variants [Internet]. [cited 2021 Jan 15]. Available from: <https://www.who.int/csr/don/31-december-2020-sars-cov2-variants/en/>
7. Peacock TP, Goldhill DH, Zhou J, Baillon L, Frise R, Swann OC, et al. The furin cleavage site of SARS-CoV-2 spike protein is a key determinant for transmission due to enhanced replication in airway cells. *bioRxiv* [Internet]. 2020 [cited 2021 Jan 13]; Available from: <https://doi.org/10.1101/2020.09.30.318311>
8. Chen J, Wang R, Wang M, Wei GW. Mutations Strengthened SARS-CoV-2 Infectivity. *J Mol Biol*. 2020;432(19):5212–26.
9. Horby P., Huntley C, Davies N, Edmunds J, Ferguson N, et al. NERVTAG note on 20I/501Y.V1 severity. SAGE [Internet]. 2021;(January). Available from: https://assets.publishing.service.gov.uk/government/uploads/system/uploads/attachment_data/file/955239/NERVTAG_paper_on_variant_of_concern_VOC_20I/501Y.V1.pdf
10. WHO. COVID-19 Weekly Epidemiological Update. World Heal Organ. 2021;(January):1;3. Available from: [Weekly epidemiological update - 19 January 2021 \(who.int\)](https://www.who.int/emergencies/diseases/novel-coronavirus-2019/weekly-epidemiological-update)