

Primerdesign™ Ltd

GMO event quantification

FMV 35S promoter

Detection and quantification of
GMO integration events by real-time PCR

100 tests

G E N E S I G

Kits by Primerdesign

Kit contents

- **FMV-GM primer/probe mix (100 reactions BROWN)**
- **FMV-WT primer/probe mix (100 reactions BROWN)**
- **Internal extraction control primer/probe mix (150 reactions BROWN)**
- **Internal extraction control template (100 reactions BLUE)**
- **Positive control (RED)**
- **RNase/DNase free water (WHITE)**
for resuspension of primer/probe mixes
- **Template preparation buffer (YELLOW)**
for resuspension of internal control template and positive control template

Reagents and equipment to be supplied by user

- **Real-time PCR Instrument**
- **oasig™ Lyophilised or Precision®PLUS 2X qPCR Master Mix**
This kit is intended for use with oasig or PrecisionPLUS 2X qPCR Master Mix.
- **Pipettes and Tips**
- **Vortex and centrifuge**
- **Thin walled 0.2 ml PCR reaction tubes**

Kit storage and stability

This kit is stable at room temperature but should be stored at -20°C on arrival. Once the lyophilised components have been resuspended they should not be exposed to temperatures above -20°C for longer than 30 minutes at a time and unnecessary repeated freeze/thawing should be avoided. The kit is stable for six months from date of resuspension under these circumstances.

Suitable sample material

All kinds of sample material suited for PCR amplification can be used. Please ensure the samples are suitable in terms of purity, concentration and DNA integrity. Always run at least one negative control with the samples. To prepare a negative control, replace the test sample DNA with RNase/DNase free water.

Notices and disclaimers

This product is developed, designed and sold for research purposes only. It is not intended for human diagnostic or drug purposes or to be administered to humans unless clearly expressed for that purpose by the Food and Drug Administration in the USA or the appropriate regulatory authorities in the country of use. During the warranty period Primerdesign genesig detection kits allow precise and reproducible data recovery combined with excellent sensitivity. For data obtained by violation to the general GLP guidelines and the manufacturer's recommendations the right to claim under guarantee is expired. PCR is a proprietary technology covered by several US and foreign patents. These patents are owned by Roche Molecular Systems Inc. and have been sub-licensed by PE Corporation in certain fields. Depending on your specific application you may need a license from Roche or PE to practice PCR. Additional information on purchasing licenses to practice the PCR process may be obtained by contacting the Director of Licensing at Roche Molecular Systems, 1145 Atlantic Avenue, Alameda, CA 94501 or Applied Biosystems business group of the Applied Biosystems Corporation, 850 Lincoln Centre Drive, Foster City, CA 94404. In addition, the 5' nuclease assay and other homogeneous amplification methods used in connection with the PCR process may be covered by U.S. Patents 5,210,015 and 5,487,972, owned by Roche Molecular Systems, Inc, and by U.S. Patent 5,538,848, owned by The Perkin-Elmer Corporation.

Trademarks

Primerdesign™ is a trademark of Primerdesign Ltd.

genesig® is a registered trademark of Primerdesign Ltd.

The PCR process is covered by US Patents 4,683,195, and 4,683,202 and foreign equivalents owned by Hoffmann-La Roche AG. BI, ABI PRISM®, GeneAmp® and MicroAmp® are registered trademarks of the Applied Biosystems (Applied Biosystems Corporation). BIOMEK® is a registered trademark of Beckman Instruments, Inc.; iCycler™ is a registered trademark of Bio-Rad Laboratories, Rotor-Gene is a trademark of Corbett Research. LightCycler™ is a registered trademark of the Idaho Technology Inc. GeneAmp®, TaqMan® and AmpliTaqGold® are registered trademarks of Roche Molecular Systems, Inc., The purchase of the Primerdesign™ reagents cannot be construed as an authorization or implicit license to practice PCR under any patents held by Hoffmann-LaRoche Inc.

Principles of the test

The kit provides a method for detecting gene insertion events by real-time PCR. The kit is based on the PCR amplification and detection of the Figwort mosaic virus (FMV) promoter. This promoter is preferred above other potential promoters because it is highly transcriptionally active and is not greatly influenced by environmental conditions or tissue types.

Real-time PCR

The primer and probe mixes provided exploit the so-called TaqMan® principle. During PCR amplification, forward and reverse primers hybridize to the sample DNA. Fluorogenic probes are included in the reaction mixtures which consists of a DNA probe labeled with a 5`-dye and a 3`-quencher. During PCR amplification, the probe is cleaved and the reporter dye and quencher are separated. The resulting increase in fluorescence can be used to detect genetically modified DNA present in the sample.

Control primers and probes

Since FMV is naturally found in the soil, it is necessary to exclude false positive results by proving that the wild type virus has not infected or contaminated a non GM sample. This kit provides control primers and probe that detect a region of the FMV genome that is not used in the genetic modification of plants.

Positive control

The kit provides a positive control for all primer and probe sets in the kit. This is a vector that contains the cloned amplicon for each primer and probe set. The one positive control is therefore used for all primer and probe sets in the kit.

Each time the kit is used, at least one positive control reaction must be included in the run. A positive result indicates that the primers and probes for detecting the FMV target worked properly in that particular experimental scenario. If a negative result is obtained the test results are invalid and must be repeated. Care should be taken to ensure that the positive control does not contaminate any other kit component which would lead to false positive results. This can be achieved by handling this component in a Post PCR environment. Care should also be taken to avoid cross-contamination of other samples when adding the positive control to the run. This can be avoided by sealing all other samples and negative controls before pipetting the positive control into the positive control well.

Negative control

To validate any positive findings, a negative control reaction should be included every time the kit is used. For this reaction the RNase/DNase free water should be used instead of template. A negative result indicates that the reagents have not become contaminated while setting up the run.

Internal extraction control

When performing DNA extraction, it is often advantageous to have an exogenous source of DNA template that is spiked into the lysis buffer. This control DNA is then co-purified with the sample DNA and can be detected as a positive control for the extraction process. Successful co-purification and qPCR amplification of the control DNA also indicates that PCR inhibitors are not present at a high concentration.

A separate primer and probe mix are supplied with this kit to detect the exogenous DNA using qPCR. The primers are present at PCR limiting concentrations which allows multiplexing with the target sequence primers. Amplification of the control DNA does not interfere with detection of the target DNA even when present at low copy number. The Internal control is detected through the **VIC** channel and gives a C_q value of 28+/-3.

Resuspension protocol

To minimise the risk of contamination with foreign DNA, we recommend that all pipetting be performed in a PCR clean environment. Ideally this would be a designated PCR lab or PCR cabinet. Filter tips are recommended for all pipetting steps.

1. Pulse-spin each tube in a centrifuge before opening

This will ensure the lyophilised primer/probe mix is in the base of the tube and is not spilt upon opening the tube.

2. Resuspend the primer/probe mixes in the RNase/DNase free water supplied, according to the table below:

To ensure complete resuspension, vortex each tube thoroughly.

Component – Resuspend in water	Volume
Pre-PCR pack	
FMV-GM DNA primer/probe mix (BROWN)	110 µl
FMV-WT DNA primer/probe mix (BROWN)	110 µl
Internal control primer/probe mix (BROWN)	165 µl

3. Resuspend the internal control template and positive control template in the template preparation buffer supplied, according to the table below:

To ensure complete resuspension, vortex each tube thoroughly.

Component – Resuspend in template preparation buffer	Volume
Pre-PCR heat-sealed foil	
Internal extraction control template (BLUE)	600 µl
Post-PCR heat-sealed foil	
Positive Control Template (RED) *	500 µl

* This component contains a high copy number template and is a VERY significant contamination risk. It must be opened and handled in a separate laboratory environment, away from the other components.

DNA extraction

The internal extraction control DNA can be added either to the DNA lysis/extraction buffer or to the DNA sample once it has been resuspended in lysis buffer.

DO NOT add the internal extraction control DNA directly to the unprocessed biological sample as this can lead to degradation and a loss in signal.

1. Add 4µl of Internal extraction control DNA (**BLUE**) to each sample in DNA lysis/extraction buffer.
2. Complete DNA extraction according to the manufacturer's protocols.

qPCR detection protocol

1. Prepare complete reaction mixes for each target primer/probe mix according to the table below:

Include sufficient reactions for positive and negative controls as well as each sample.

Component	1 reaction
oasig or PrecisionPLUS 2X qPCR Master Mix	10 μ l
WT or GM primer/probe mix (BROWN)	1 μ l
Internal extraction control primer/probe mix (BROWN)	1 μ l
RNase/DNase free water (WHITE)	3 μ l
Final volume	15 μl

2. Pipette 15 μ l of each mix into individual wells according to your qPCR experimental plate set up.

3. Prepare sample DNA templates for each of your samples.

4. Pipette 5 μ l of DNA template into each well, according to your experimental plate set up.

For negative control wells use 5 μ l of RNase/DNase free water. The final volume in each well is 20 μ l.

5. Pipette 5 μ l of positive control template into the positive control wells.

The final volume in each well is 20 μ l

qPCR amplification protocol

Amplification conditions using oasig or PrecisionPLUS 2X qPCR Master Mix

	Step	Time	Temp
Cycling x50	Enzyme activation	2 min	95°C
	Denaturation	10 s	95°C
	DATA COLLECTION*	60 s	60°C

*Fluorogenic data should be collected during this step through the FAM and VIC channels.

Interpretation of results


Results from both the GM and WT target can be analysed using the table below to determine whether a result can be called as positive or negative.

Target (FAM)	Internal control (VIC)	Positive control	Negative control	Interpretation
≤ 30	+/-	+	-	POSITIVE QUANTITATIVE RESULT calculate copy number
> 30	+	+	-	POSITIVE QUANTITATIVE RESULT calculate copy number
> 30	-	+	-	POSITIVE QUALITATIVE RESULT do not report copy number as this may be due to poor sample extraction
-	+	+	-	NEGATIVE RESULT


+/-	+/-	+	≤ 35	EXPERIMENT FAILED due to test contamination
+/-	+/-	+	> 35	*
-	-	+	-	SAMPLE PREPARATION FAILED
+/-	+/-	-	+/-	EXPERIMENT FAILED

Positive control template (**RED**) is expected to amplify between Cq 16 and 23. Failure to satisfy this quality control criterion is a strong indication that the experiment has been compromised.

*Where the test sample is positive and the negative control is positive with a Cq > 35, the sample must be reinterpreted based on the relative signal strength of the two results:

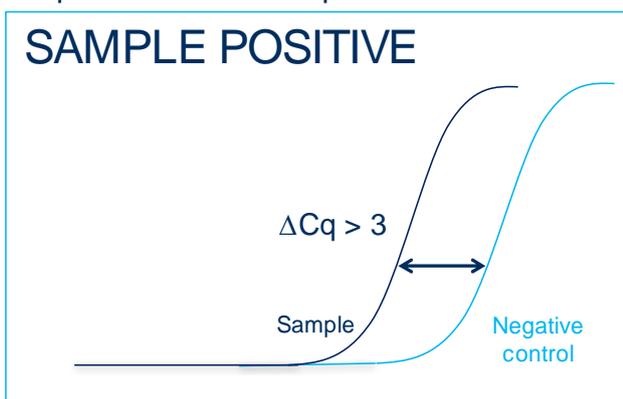


If the sample amplifies > 3 Cq earlier than the negative control then the sample should be reinterpreted (via the table above) with the negative control verified as negative.

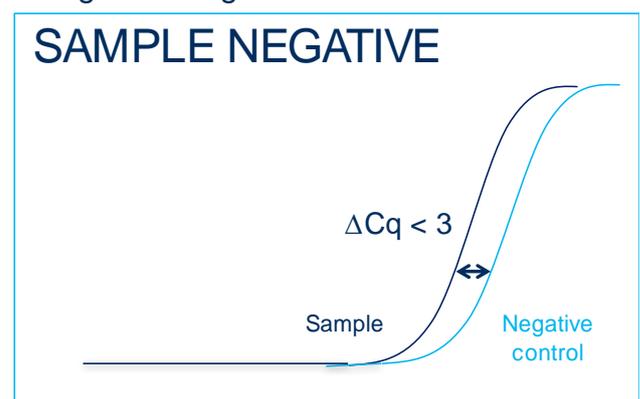


If the sample amplifies < 3 Cq earlier than the negative control then the positive sample result is invalidated and a negative call is the correct result.

Once results for both the GM and WT target have been analysed individually using the table on the previous page, these results may be used to determine the presence of a genetically modified sample using the following table:

GM Result	WT Result	Decision
POSITIVE RESULT	NEGATIVE RESULT	Significant presence of genetically modified material in tested sample
NEGATIVE RESULT	POSITIVE RESULT	No significant presence of genetically modified material in the tested sample
NEGATIVE RESULT FOR BOTH TARGETS		No significant presence of genetically modified material in the tested sample
POSITIVE RESULT FOR BOTH TARGETS		Where a positive signal is obtained with both the GM and the FMV-WT primer/probe sets, this indicates that both naturally occurring and GM FMV is present in the samples. The data must be carefully considered by looking at the relative signal strength of the two results to determine if the GM material is present at significant level.

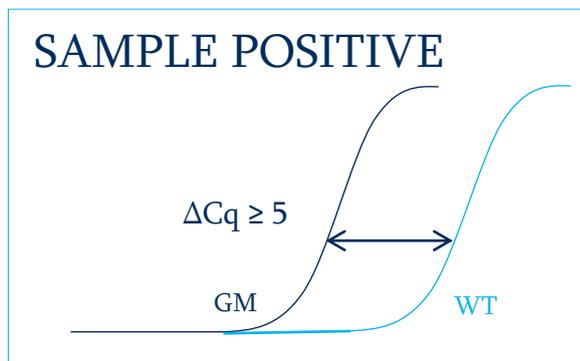

If the GM primer/probe amplifies $\geq 5Cq$ values earlier than the WT control primer/probe, then the test confirms the presence of both the FMV organism and GM plant material.

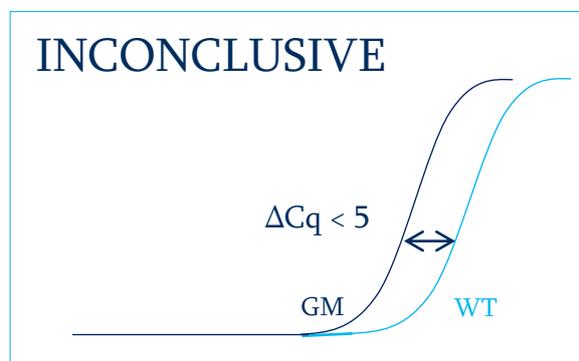

If the traces for the WT and GM are closer together with a $< 5Cq$ difference, then the test is indeterminate since the presence of WT FMV prevents the analysis of the GM content of the sample.